

HPLC PURITY REPORT

MOTS-c

Lot 20260123

MANUFACTURE DATE
January 23, 2026

ANALYSIS DATE
January 23, 2026

REPORTED PURITY
≥98.0%

DOCUMENT TYPE
HPLC Purity Report

This document is provided as part of Kodiak's lab transparency archive. It accompanies a research-use-only compound and reflects vendor analytical documentation. Independent third-party verification by Janoshik Analytical is performed on rotating samples and archived alongside vendor reports.

The following pages reproduce the original report as received from the manufacturer or analytical laboratory. No content has been altered.


ARCHIVE REFERENCE
kodiak-hplc-mots-c-20260123.pdf

PUBLISHED BY
kodiak.org

Single Injection Report



Data file:	2026-01-23 15-52-56+08-00-29.dx		
Sequence Name:	20260123-1	Project Name:	A
Sample name:	DZT-034 2.02MG/ML	Operator:	System
Instrument:	Agilent1260	Injection date:	2026-01-23 15:53:44+08:00
Inj. volume:	5.000	Location:	P1-F7
Acq. method:	25-50.amx	Type:	Sample
Processing method:	GC_LC_DefaultMethod.pmx	Sample amount:	0.00
Manually modified:	Manual Integration		

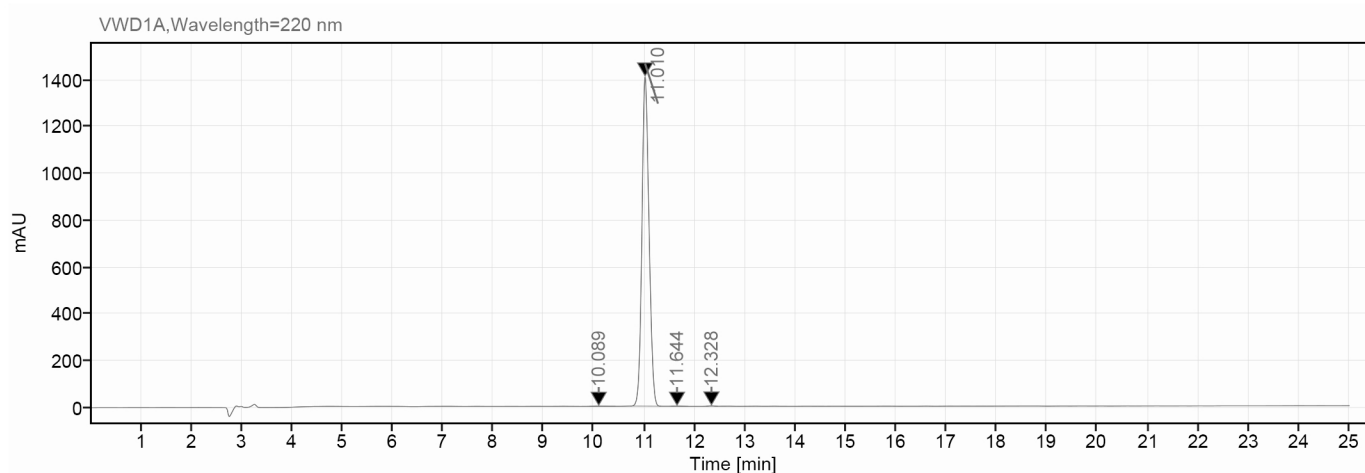

Signal: VWD1A,Wavelength=220 nm

RT [min]	Type	Width [min]	Area	Height	Area%	Name
10.089	MM m	0.52	13.35	0.98	0.10	
11.010	MM m	0.60	13860.30	1408.46	99.74	
11.644	MM m	0.35	8.34	0.81	0.06	
12.328	MM m	0.23	14.17	2.06	0.10	
Sum			13896.15			