

HPLC PURITY REPORT

Selank

Lot 20260313

MANUFACTURE DATE

March 13, 2026

ANALYSIS DATE

March 14, 2026

REPORTED PURITY

99.45%

DOCUMENT TYPE

HPLC Purity Report

This document is provided as part of Kodiak's lab transparency archive. It accompanies a research-use-only compound and reflects vendor analytical documentation. Independent third-party verification by Janoshik Analytical is performed on rotating samples and archived alongside vendor reports.

The following pages reproduce the original report as received from the manufacturer or analytical laboratory. No content has been altered.

ARCHIVE REFERENCE

kodiak-hplc-selank-20260313.pdf

PUBLISHED BY

kodiak.org

<sample>

Sample Information

Acquired by

Sample Name

Sample ID

Tray#

Vial#

Injection Volume

Data File

Method File

Batch File

Report Format File

Date Acquired

Date Processed

: System Administrator

: DZT-043 2.30MG/ML

: 20260313-01

: 1

: 39

: 10

: DZT-043 20260313-01.lcd

: 8-33.lcm


: 20260313-01.lcb

: Enginsh Report Format.lsr

: 2026/3/13 14:01:10

: 2026/3/13 14:27:37

<HPLC>

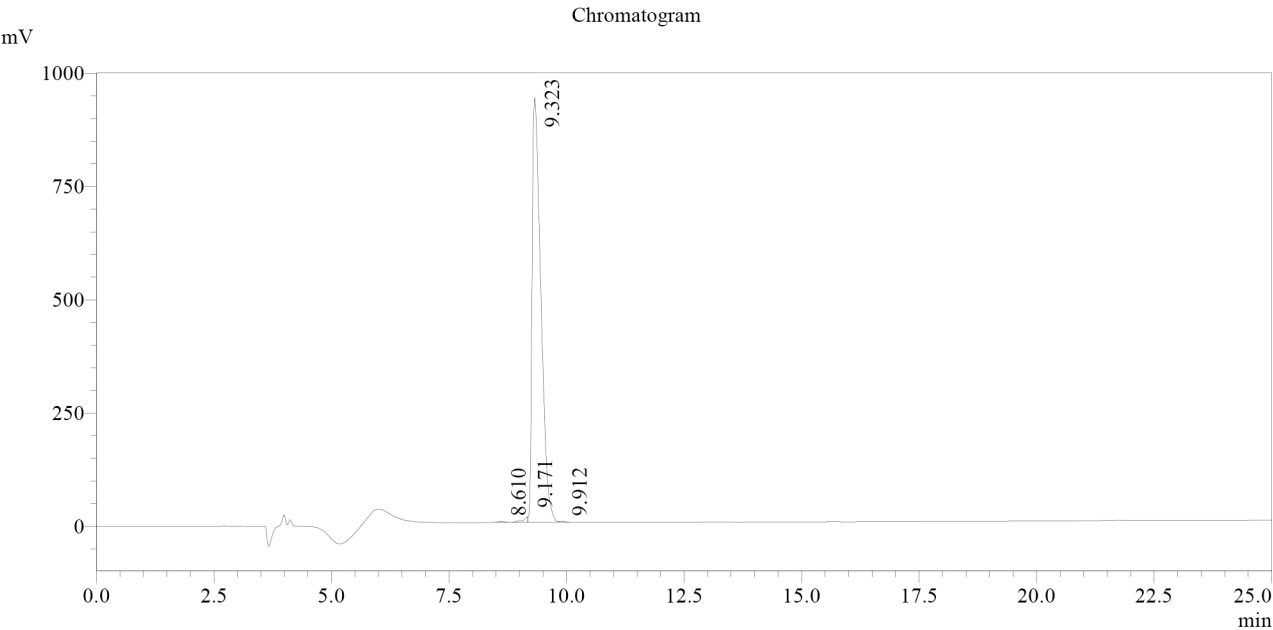

<Peak Table>

Peak Table

Detector A 220nm

Peak#	Ret. Time	Height	Area	Area%	Width at 50% Height
1	8.610	1496	14106	0.115	0.158
2	9.171	11407	81695	0.667	--
3	9.323	936658	12126649	99.081	0.204
4	9.912	2390	16662	0.136	--
Total		951952	12239112	100.000	