

Kodiak

LAB RESULTS

MASS SPECTROMETRY REPORT

Semax

Lot 20260331

MANUFACTURE DATE

March 31, 2026

ANALYSIS DATE

April 1, 2026

REPORTED PURITY

99.75% (HPLC: 99.76%)

DOCUMENT TYPE

Mass Spectrometry Report

This document is provided as part of Kodiak's lab transparency archive. It accompanies a research-use-only compound and reflects vendor analytical documentation. Independent third-party verification by Janoshik Analytical is performed on rotating samples and archived alongside vendor reports.

The following pages reproduce the original report as received from the manufacturer or analytical laboratory. No content has been altered.


ARCHIVE REFERENCE

kodiak-ms-semax-20260331.pdf

PUBLISHED BY

kodiak.org

MASS SPECTROMETRY REPORT

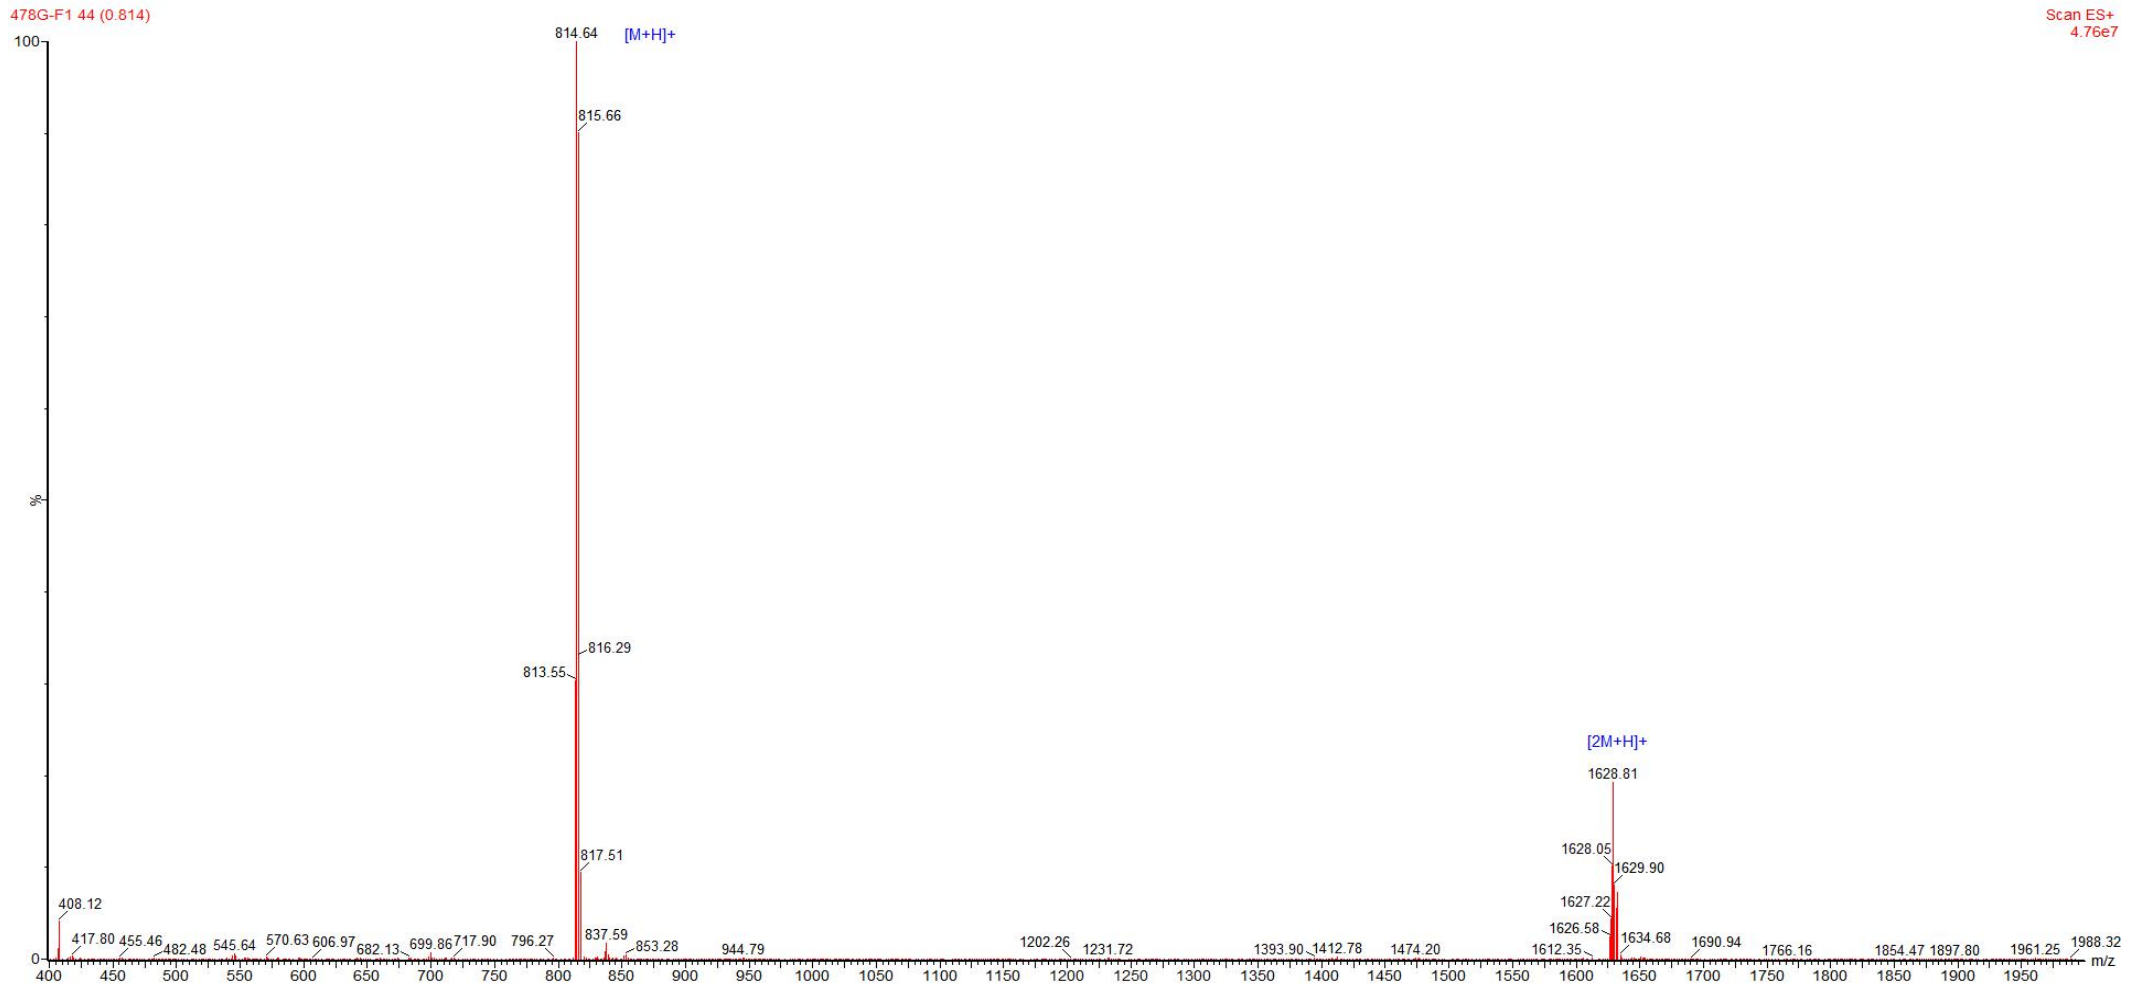

Sample Description

Analyzed date: 2026-03-31
Analyst: PY
Sample: DZT-044
M.W.: 813.92
Lot. No.: 20260331-02

Instrument

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Waters ZQ2000

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H₂O/50%ACN